



MAGLUMI[®] X Series

Fully-auto Chemiluminescence Immunoassay System

**All Balance
and
Strong**



MAGLUMI® X3

Save Your Space without Compromise

Compatible with Small and Medium-sized Hospitals and Labs

200

Tests/Hour

< 0.68m²

Space
Occupied



80

Incubation
Positions

20

Reagent
Positions

72

Sample
Positions

Small but strong

- The throughput per unit area is 294 T/h/m²
- Compatible with all MAGLUMI® reagents with perfect compatibility (211 parameters)

Low failure rate and accurate result

- Reaction cup can avoid light pollution, ensuring the accuracy of results
- Integrated packaging of cuvette to avoid the stuck, blockage and scratches
- TEFLON-coated pipetting needle is equipped with independent washing unit to avoid carry-over, ensuring accurate results

Excellent performance

- The comprehensive advanced design of MAGLUMI® X3 ensures excellent performance, such as the latest intelligent washing technology and bidirectional temperature control measurement

Convenient and efficient

- No-pause loading/unloading of reagents/samples/reaction cups without waiting or interrupting tests
- Intuitive indicator lights make no need to check reagents and consumables frequently


Cost-efficient and intelligent

- Saving consumable costs by not using disposable Tips
- Pipetting needle with three error detection technologies (liquid level /clot /crash), reducing error rate

MAGLUMI® X6

Flexible Combination Meeting Various Needs

Targeted for Medium/High-volume Laboratory

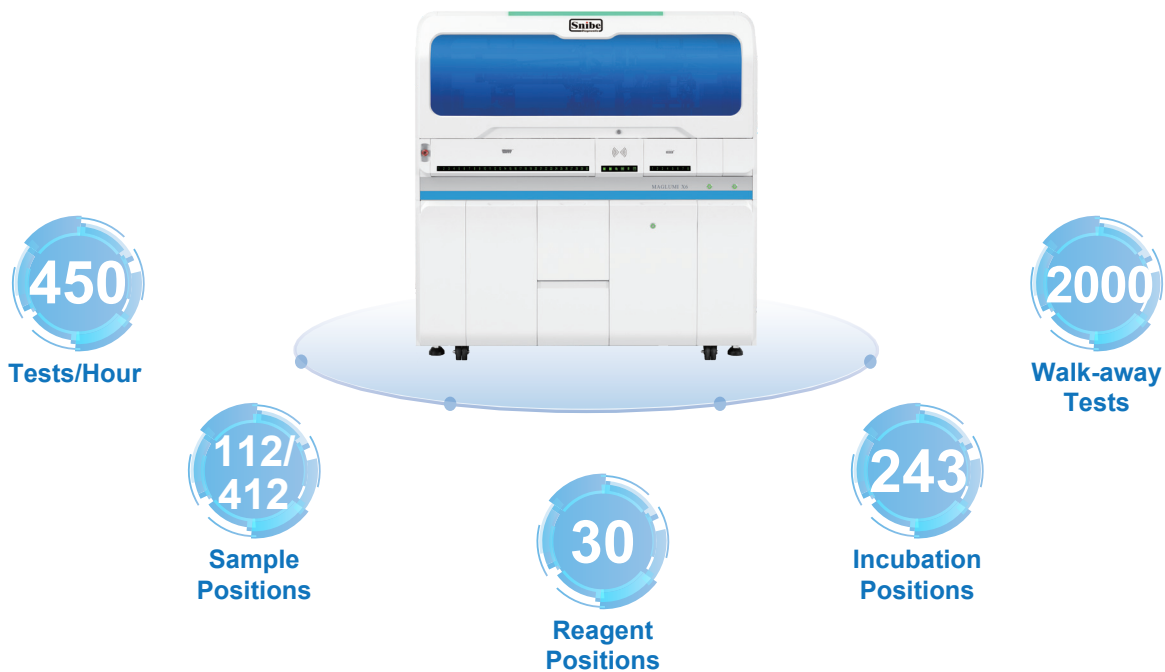

Fast and cost-efficient

- 450 T/H with mid-size, suitable for medium or high-volume laboratory
- Compatible with all MAGLUMI® reagents with perfect compatibility (211 parameters)

Convenience and high efficiency

- No-pause loading/unloading reagents/samples/consumables without interrupting tests
- One-stop, one-side operation saving space and steps
- Intelligent SnibeLinker® remote service solution to ensure the fast response

Flexible combination according to requirements

- Additional sample positions available that sample positions can expand to 412
- Capable to link Total Laboratory Automation System (TLA)

User-friendly design

- Up to 2000 walk-away tests to avoid high frequency of manual intervention
- Dual-mode wash liquid preparation—automatic or manual
- Intelligent UI interface, user-friendly, easy and convenient operation


Advanced and accurate function

- A revolutionary pipetting volume from 10 μL to 280 μL with higher accuracy and low pipetting CV
- Four kinds of pipetting error detection technologies reduce sampling error rate

MAGLUMI® X8

Super-high Throughput CLIA Solution

Targeted for Large Labs, Chain Labs and Hospitals

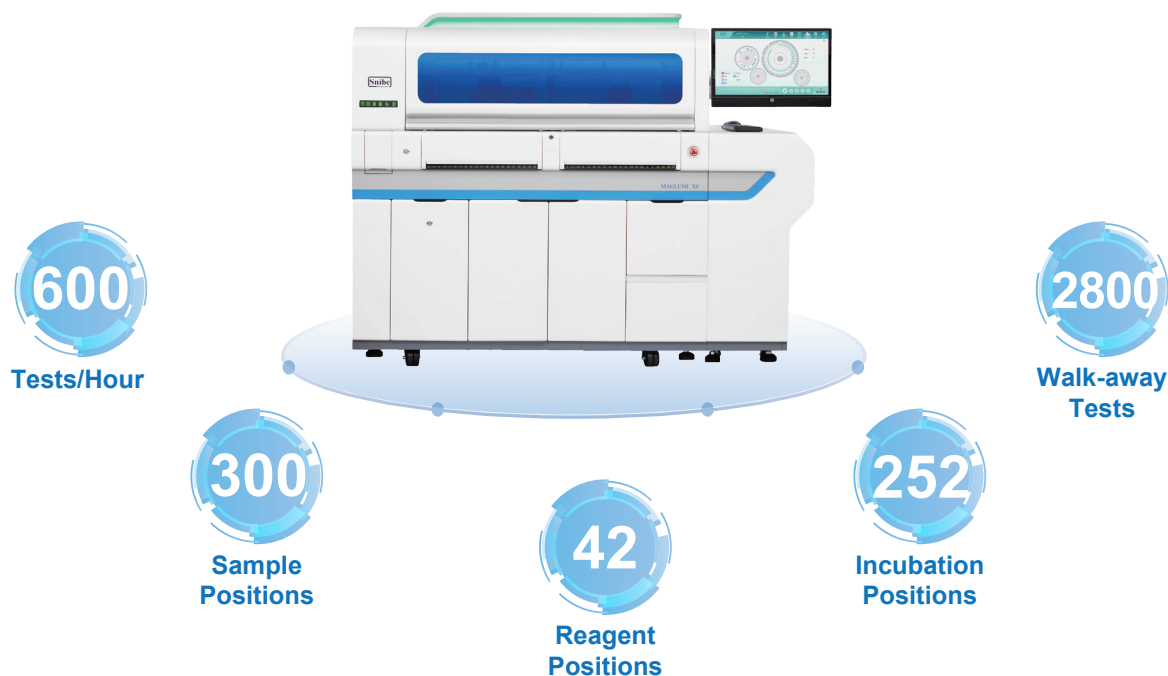

Excellent performance

- One of the fastest CLIA analyzers with 600 T/H (Single module)
- Up to 2400 T/H (Four modules combined)
- Compatible with all MAGLUMI® reagents with perfect compatibility (211 parameters)

Saving manpower

- Long walk-away time—2800 tests, saving human labor greatly
- 2912 cuvettes loading in one time with fully cuvette loader, no need to add frequently

Advanced intelligence

- Capable to link Laboratory Automation system (TLA/LAS)
- Capable to integrate with Biossays® C8 (high-throughput chemistry analyzer) and decapper module

Considerate design

- Multidimensional indicator lights, real-time monitoring the status of analyzer from a distance
- Dual-mode wash liquid preparation—automatic or manual
- Automatic reagent cover plate and double temperature mode reducing reagent volatilization and enhancing the stability of reagent kits on board



Convenient operation

- User-friendly interface, easy and convenient operation
- No-pause loading/unloading reagents/samples/consumables without interrupting tests

Outstanding Technologies — X-tech

■ Pioneer in Optional Wash Liquid Preparation*

Dual-mode wash liquid preparation—Automatic or Manual

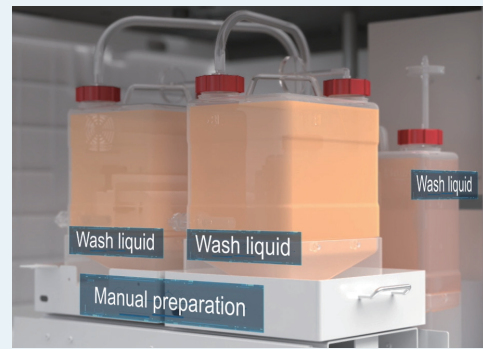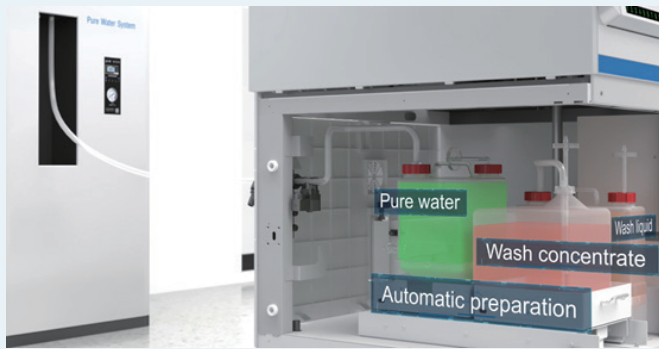


- Select Auto mode on the software, connect the X6/X8 to the water purification system, minimize your operational burden
- If water purification system is not available, the preparation can be done by manually mixing the wash liquid with pure water

■ Flexible Expansion Solutions*



- Same modules combined with high throughput and small space occupation
- Capable to integrate with **Biossays® C8** (High-throughput Chemistry Analyzer)
- Capable to connect with decapper module

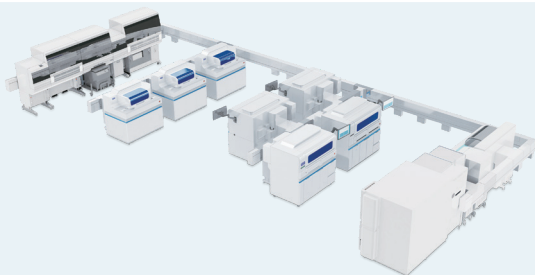

- Capable to link laboratory automation system (TLA/LAS)

* For X6 and X8

Key Technologies

CLIA uses two important technologies, one is the labelling technology which determines the reaction mode, and the other is a separation technology which determines the sensitivity, accuracy and precision of the reagents.


■ Labelling Technology

The **MAGLUMI®** system applies ABEI labels. ABEI is a non-enzyme small molecule with special molecular formula to enhance stability in acid and alkaline buffer. Using fast Chemiluminescence, ABEI's chemical reaction with sodium hydroxide (NaOH) and Hyperoxide (H_2O_2) finishes the process in 3 seconds.

■ Separation Technology

MAGLUMI® uses Magnetic Microbeads. As separation technology, it has been widely used in the field of CLIA. Compared with traditional separation technology, it has the following advantages:

- Shortening the reaction time by enlarging the reaction area of antigens and antibodies.
- Enhancing the sensitivity by better and faster capture of antigens and antibodies.
- Reducing inter or intra-assay discrepancies significantly by mixing the reagents thoroughly in a liquid separation platform.
- Enhancing the accuracy by absorbing antigens and antibodies through chemical reaction.

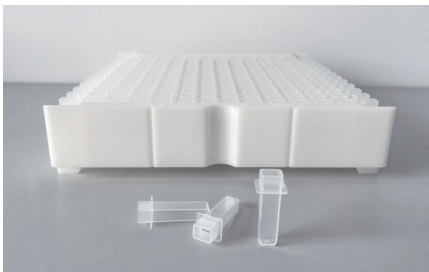

Reaction Cup



Disposal TIP



Starter 1+2



Wash Concentrate



Tubing Cleaning Solution



Light Check

Broad CLIA Test Menu with 211 Assays

Thyroid

TSH (3rd Generation)
T4
T3
FT4
FT3
Tg (Thyroglobulin)
TGA (Anti-Tg)
Anti-TPO
TRAb
TMA
Rev T3
T-Uptake

Hepatic Fibrosis

HA
PIIIP N-P
C IV
Laminin
Cholyglycine
GP73

TORCH

Toxo IgG
Toxo IgM
Rubella IgG
Rubella IgM
CMV IgG
CMV IgM
HSV-1/2 IgG
HSV-1/2 IgM
HSV-1 IgG
HSV-2 IgG
*HSV-2 IgM
*HSV-1 IgM
*Toxo IgG Avidity
*CMV IgG Avidity

STAT-X™

*hs-cTnl
*NT-proBNP
*Myoglobin
*D-dimer
*PCT
*CRP

EBV

EBV EA IgG
EBV EA IgA
EBV VCA IgG
EBV VCA IgM
EBV VCA IgA
EBV NA IgG
EBV NA IgA

Inflammation Monitoring

CRP
PCT (Procalcitonin)
IL-6 (Interleukin 6)
SAA (Serum Amyloid A)
*PCT (STAT)
*CRP (STAT)
*TNF-α

Kidney Function

β₂-MG
Albumin
*NGAL

Fertility

FSH
LH
HCG/β-HCG
PRL (Prolactin)
Estradiol
Testosterone
free Testosterone
DHEA-S
Progesterone
free Estradiol
17-OH Progesterone
AMH
SHBG
Androstenedione
PIGF
sFit-1

Autoimmune

Anti-CCP
Anti-dsDNA IgG
ANA Screen
ENA Screen
Anti-Sm IgG
Anti-Rib-P IgG
Anti-Scl-70 IgG
Anti-Centromeres IgG
Anti-Jo-1 IgG
Anti-M2-3E IgG
Anti-Histones IgG
Anti-nRNP/Sm IgG
Anti-SS-B IgG
Anti-SS-A IgG
TGA (Anti-Tg)
Anti-TPO
TRAb
TMA
ICA
IAA (Anti Insulin)
GAD 65
Anti-IA2
*ZnT8
Anti-MPO IgG
*Anti-PR3 IgG
*Anti-GBM IgG
*Anti-Cardiolipin IgG
*Anti-Cardiolipin IgM
*Anti-Cardiolipin IgA
*Anti-Cardiolipin screen
*β2-Glycoprotein I IgG
*β2-Glycoprotein I IgM
*β2-Glycoprotein I IgA
*β2-Glycoprotein I screen
*Anti-tTG IgA
*Anti-tTG IgG
*DGP IgA
*DGP IgG

Hypertension

Direct Renin
Aldosterone
Angiotensin I
Angiotensin II
Cortisol
ACTH

Immunoglobulins

IgM
IgA
IgE
IgG

Tumor Markers

AFP
CEA
Total PSA
f-PSA
CA 125
CA 15-3
CA 19-9
PAP
CA 50
CYFRA 21-1
CA 242
CA 72-4
NSE
S-100
SCCA
TPA-snibe
ProGRP
HE4
HER-2
PIVKA-II

Infectious Disease

HBsAg
Anti-HBs
HBeAg
Anti-HBe
Anti-HBc
Anti-HBc IgM
Anti-HCV
Syphilis
Anti-HAV
HAV IgM
*HEV IgG
*HEV IgM
HIV Ab/Ag Combi
Chagas
HTLV I+II
H.pylori IgG
H.pylori IgA
H.pylori IgM
2019-nCoV IgG
2019-nCoV IgM
SARS-CoV-2 S-RBD IgG
SARS-CoV-2 Neutralizing Antibody
SARS-CoV-2 Ag
Monkeypox Virus Ag
Dengue Virus IgG
Dengue Virus NS1
*Dengue Virus IgM
*Chlamydia Pneumoniae IgG
*Chlamydia Pneumoniae IgM
*Mycoplasma Pneumoniae IgG
*Mycoplasma Pneumoniae IgM

Veterinary Testing

*cTSH
*cTT4
*vFT4

Glyco Metabolism

C-Peptide
Insulin
GAD 65
Anti-IA2
ICA
IAA (Anti Insulin)
Proinsulin
*Glucagon
*ZnT8

Cardiac

CK-MB
Troponin I
Myoglobin
hs-cTnl
hs-CRP
H-FABP
NT-proBNP
BNP
D-Dimer
Lp-PLA2
MPO
HCY
*hs-cTnl (STAT)
*NT-proBNP (STAT)
*Myoglobin (STAT)
*D-dimer (STAT)

Coagulation Markers

D-Dimer
*TAT
*TM
*PIC
*tPAIC

Metabolism

Pepsinogen I
Pepsinogen II
Gastrin-17
GH (hGH)
IGF-I
IGFBP-3

Prenatal Screening

AFP (Prenatal Screening)
free β-HCG
PAPP-A
free Estradiol

Anemia

Vitamin B12
Ferritin
Folate (FA)
EPO
RBC Folate

Drug Monitoring

Digoxin
CSA (Cyclosporine A)
FK 506 (Tacrolimus)

Bone Metabolism

Calcitonin
Osteocalcin
25-OH Vitamin D
Intact PTH
β-CTx
total P1NP

*Available soon



MAGLUMI® , Snibelis™ and SnibeLinker™ are trademarks of Snibe.
All other product names and trademarks are the property of their respective owners.



Shenzhen New Industries Biomedical Engineering Co., Ltd.
(SNIBE Co.,Ltd.)

No.23, Jinxiu East Road, Pingshan District, 518122 Shenzhen,
P.R. China

Tel: +86 755 26501514
Email: sales@snibe.com

Fax: +86 755 26654850
Web: www.snibe.com

Follow us on

